

A.A. Jansson

2070 Airport Rd
 Waterford, MI 48327
 Phone No. 248-674-4811 - Fax No. 248-674-1234

Certificate of Calibration

Web page: www.aaajansson.com



Company: DIGIPAS TECHNOLOGIES INC.
Address: 200 SPECTRUM CENTER DRIVE
 SUITE 300
 IRVINE, CA 92618
Contact:
Job #: 66336-1

Doc #: 142654
Calibration Date: 1/2/2024
PO/Acct: DPO23-0050
Page: 1 of 3
Visual Condition: GOOD
Date Received: 12/5/2023

Gage Type: DIGITAL LEVEL
Mfg: DIGIPAS
Procedure: AAJ CM-51.0


Cert No.: DIG12A29737
Model: DWL5800XY
Serial #: 12A29737

+ / - Tolerances: +3.000000 / -3.000000
Graph Scale: +0.200000

X AXIS (+) SLOPE

Nominal	Actual	Deviation
+825.000000	+825.000000	+0.000000
+1650.000	+1650.000	+0.000000
+2476.000	+2479.000	+3.000000
+3300.000	+3302.000	+2.000000
+4125.000	+4127.000	+2.000000
+4949.000	+4950.000	+1.000000
+6186.000	+6189.000	+3.000000

Measurement Uncertainty: ± 6 ARC SECONDS

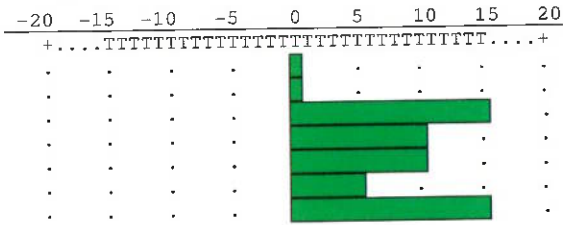


+ / - Tolerances: +3.000000 / -3.000000
Graph Scale: +0.200000

X AXIS (-) SLOPE

Nominal	Actual	Deviation
+825.000000	+825.000000	+0.000000
+1650.000	+1651.000	+1.000000
+2476.000	+2478.000	+2.000000
+3300.000	+3302.000	+2.000000
+4125.000	+4127.000	+2.000000
+4949.000	+4950.000	+1.000000
+6186.000	+6189.000	+3.000000

Measurement Uncertainty: ± 6 ARC SECONDS

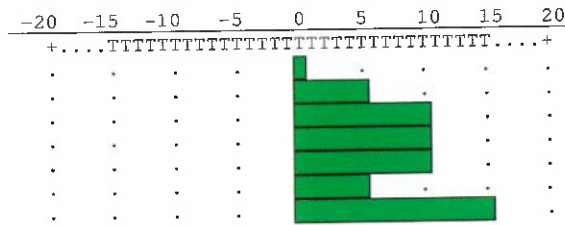


+ / - Tolerances: +3.000000 / -3.000000
Graph Scale: +0.200000

DUAL AXIS X (+) SLOPE

Nominal	Actual	Deviation
+825.000000	+826.000000	+1.000000
+1650.000	+1651.000	+1.000000
+2476.000	+2479.000	+3.000000
+3300.000	+3302.000	+2.000000
+4125.000	+4127.000	+2.000000
+4949.000	+4951.000	+2.000000


Measurement Uncertainty: ± 6 ARC SECONDS

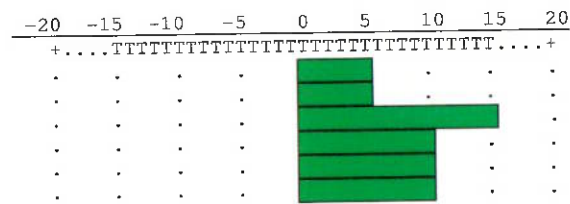

+ / - Tolerances: +3.000000 / -3.000000
Graph Scale: +0.200000

DUAL AXIS X (-) SLOPE

Nominal	Actual	Deviation
+825.000000	+826.000000	+1.000000
+1650.000	+1651.000	+1.000000
+2476.000	+2479.000	+3.000000
+3300.000	+3302.000	+2.000000
+4125.000	+4127.000	+2.000000
+4949.000	+4951.000	+2.000000

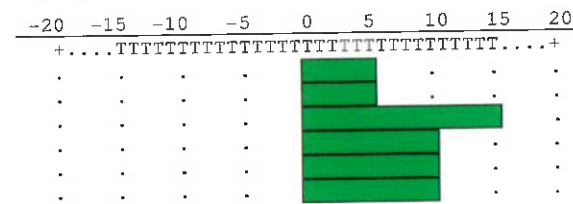

A.A. Jansson

2070 Airport Rd
Waterford, MI 48327

Phone No. 248-674-4811 - Fax No. 248-674-1234

Certificate of Calibration

Web page: www.ajansson.com

Page #: 2 of 3
Gage Type: DIGITAL LEVEL
Mfg: DIGIPAS
Procedure: AAJ CM-51.0

Doc #: 142654
Cert No.: DIG12A29737
Model: DWL5800XY
Serial #: 12A29737


Measurement Uncertainty: ± 6 ARC SECONDS

+ / - Tolerances: +3.000000 / -3.000000
Graph Scale: +0.200000

DUAL AXIS Y (+) SLOPE

Nominal	Actual	Deviation
+825.000000	+825.000000	+0.000000
+1650.000	+1650.000	+0.000000
+2476.000	+2478.000	+2.000000
+3300.000	+3303.000	+3.000000
+4125.000	+4127.000	+2.000000
+4949.000	+4949.000	+0.000000

Measurement Uncertainty: ± 6 ARC SECONDS

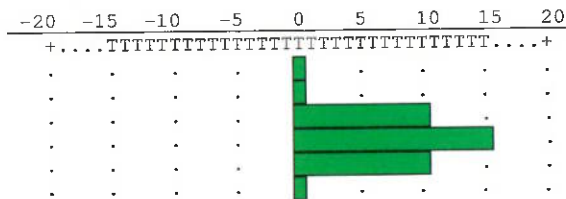


+ / - Tolerances: +3.000000 / -3.000000
Graph Scale: +0.150000

DUAL AXIS Y (-) SLOPE

Nominal	Actual	Deviation
+825.000000	+824.000000	-1.000000
+1650.000	+1651.000	+1.000000
+2476.000	+2478.000	+2.000000
+3300.000	+3302.000	+2.000000
+4125.000	+4127.000	+2.000000
+4949.000	+4950.000	+1.000000

Measurement Uncertainty: ± 6 ARC SECONDS

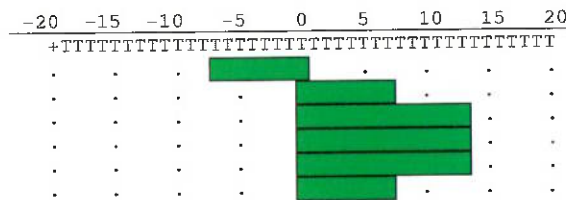

Comments:

CLEANED CALIBRATED AND CERTIFIED
DATA IS REPORTED IN ARC SECONDS
TEMPERATURE: 68.17° F
HUMIDITY: 29.4%
MANUFACTURER TOLERANCE:
 ± 1 ARC SECOND (0-1080 ARC SECOND)
 ± 3 ARC SECONDS FOR ALL OTHER ANGLES
CERTIFICATE ISSUE DATE: 1/4/2024

We certify the equipment used for this calibration is traceable to NIST through one or more of the following numbers:

LC-1: LEVEL FIXTURE / AMPLIFIER & PROBE
685-O-0000001278-20, 683/292348-18 Cal Date / Due Date: 12/21/2023 -- 12/21/2024
QC-SP: 5" SINE PLATE
10015087, 220551-U-1, L220826-6, L8582038580 Cal Date / Due Date: 1/31/2023 -- 1/31/2025
M-1: 97 Pcs Rect.
685-O-0000001278-20, 685-O-0000034629-21 Cal Date / Due Date: 5/4/2023 -- 5/4/2024
27124: 24" X 36" SURFACE PLATE
3829/000663/000548, 4459-2, TEMP-001 Cal Date / Due Date: 8/3/2023 -- 8/3/2024

Gage Status: PASS

Unless otherwise noted in comments the following will apply;

1. Reported readings taken at 68°F \pm 4°F Relative humidity less than 50%
2. Compliance statements will be binary and a simple acceptance decision rule will be applied, with no consideration for measurement uncertainty. The tolerance used will be per manufacturers Specification.

A.A. Jansson

Certificate of Calibration

2070 Airport Rd
Waterford, MI 48327

Phone No. 248-674-4811 - Fax No. 248-674-1234


Web page: www.aajansson.com

Page #: 3 of 3
Gage Type: DIGITAL LEVEL
Mfg: DIGIPAS
Procedure: AAJ CM-51.0

Doc #: 142654
Cert No.: DIG12A29737
Model: DWL5800XY
Serial #: 12A29737

3. This is an endorsed Calibration Certificate (A2LA 1182.01 valid until 8/31/2024) in accordance to ISO/IEC 17025:2017.
4. Data is "As-Found" and "As-Left" and item is "Used."

Reported Measurement Uncertainties are based upon a 95% confidence level, $k=2$. This report shall not be reproduced, except in full, without written permission by A.A. Jansson, Inc. The results reported relate only to the items calibrated. Any number of factors may cause the subject of this calibration to drift out of calibration before the calibration interval has expired. Calibrations performed in accordance with the A.A. Jansson, Inc. Quality Assurance Manual Revision 10, Dated May 29, 2020. We certify the equipment used for this calibration is traceable to the International System of Units (SI) via standards traceable to NIST or other National Metrology Institutes (NMI).

Certified By: Steve Wilt Signature: _____ Authorized By:  _____

Brian Lemon - Technician

This certificate is not valid unless all 3 page(s) are present.
Results of this certificate relate only to the item mentioned in document header.
END OF DOCUMENT